

Airpointer

**DTn**<sup>o</sup>

[www.dtn.com](http://www.dtn.com)





**90% smaller  
than traditional  
measurement stations**

**Flexible at  
point of interest**

**Modular  
configuration  
for each application**

**Approved compliance  
with legal standards  
(EN, US-EPA, SEPA)**

**Successful through more than  
30 years** in the industry

**80% less  
maintenance costs**

**Easy web  
browser-based  
data access**

**Turn-key product, up and running in  
30 minutes**



## Airpointer modules at a glance

The airpointer is easy to install, cost-effective to operate, and easy to maintain.

The airpointer's modular design comprising a base unit, analyzing modules and sensor modules allows for a configuration according to different application requirements.

The airpointer's compact design enables it to be installed almost everywhere. Due to its optimized thermal management, the airpointer consumes less power compared to conventional monitoring stations.

The airpointer offers a choice of analysis modules using type approved reference methods for monitoring airborne pollutants (SO<sub>2</sub>, NO<sub>2</sub>/NO<sub>x</sub>, CO, O<sub>3</sub>, and PM) classified as relevant by the EU, the WHO, the US-EPA and further responsible organizations all over the world.

With our fully integrated gas chromatograph we can measure BTX (Benzene/Toluene/Ethylbenzene/Xylene) without any carrier gas and provide daily automated calibration check.

A fast optical system or an approved PM analyzer is used for monitoring PM.

The integrated data management system records monitoring data of the airpointer's own analysis modules as well as various external third-party sensors. An internal web server enables data retrieval by using any Internet connection. Data are available worldwide via access authorization and can be presented in clearly arranged graphics. All parameters can be displayed locally or online.



**Zero air supply**  
for daily quality control for generating pollutant-free air

**PM sampling inlet**  
for continuous PM<sub>2.5</sub>, PM<sub>10</sub> or TSP measurement depending on the configuration. Temperature-controlled to avoid the effects of humidity

**Air sampling inlet**  
continuously draws in air samples according to respective directives

**Handle**

**Computer**


**Gas spring strut**

**Maintenance door**  
provides access for easy inlet filter changing, network connection, and a calibration gas inlet

**Air conditioning**  
controls the internal operation temperature to ensure measurement data quality

**Pump**  
draws sampling gas through modules using one or two pistons, depending on configuration

**Extended lifetime filter (optional)**  
A Teflon screen cylinder filter allowing for extended filter life even for high PM contamination may be used instead of the standard Teflon filter

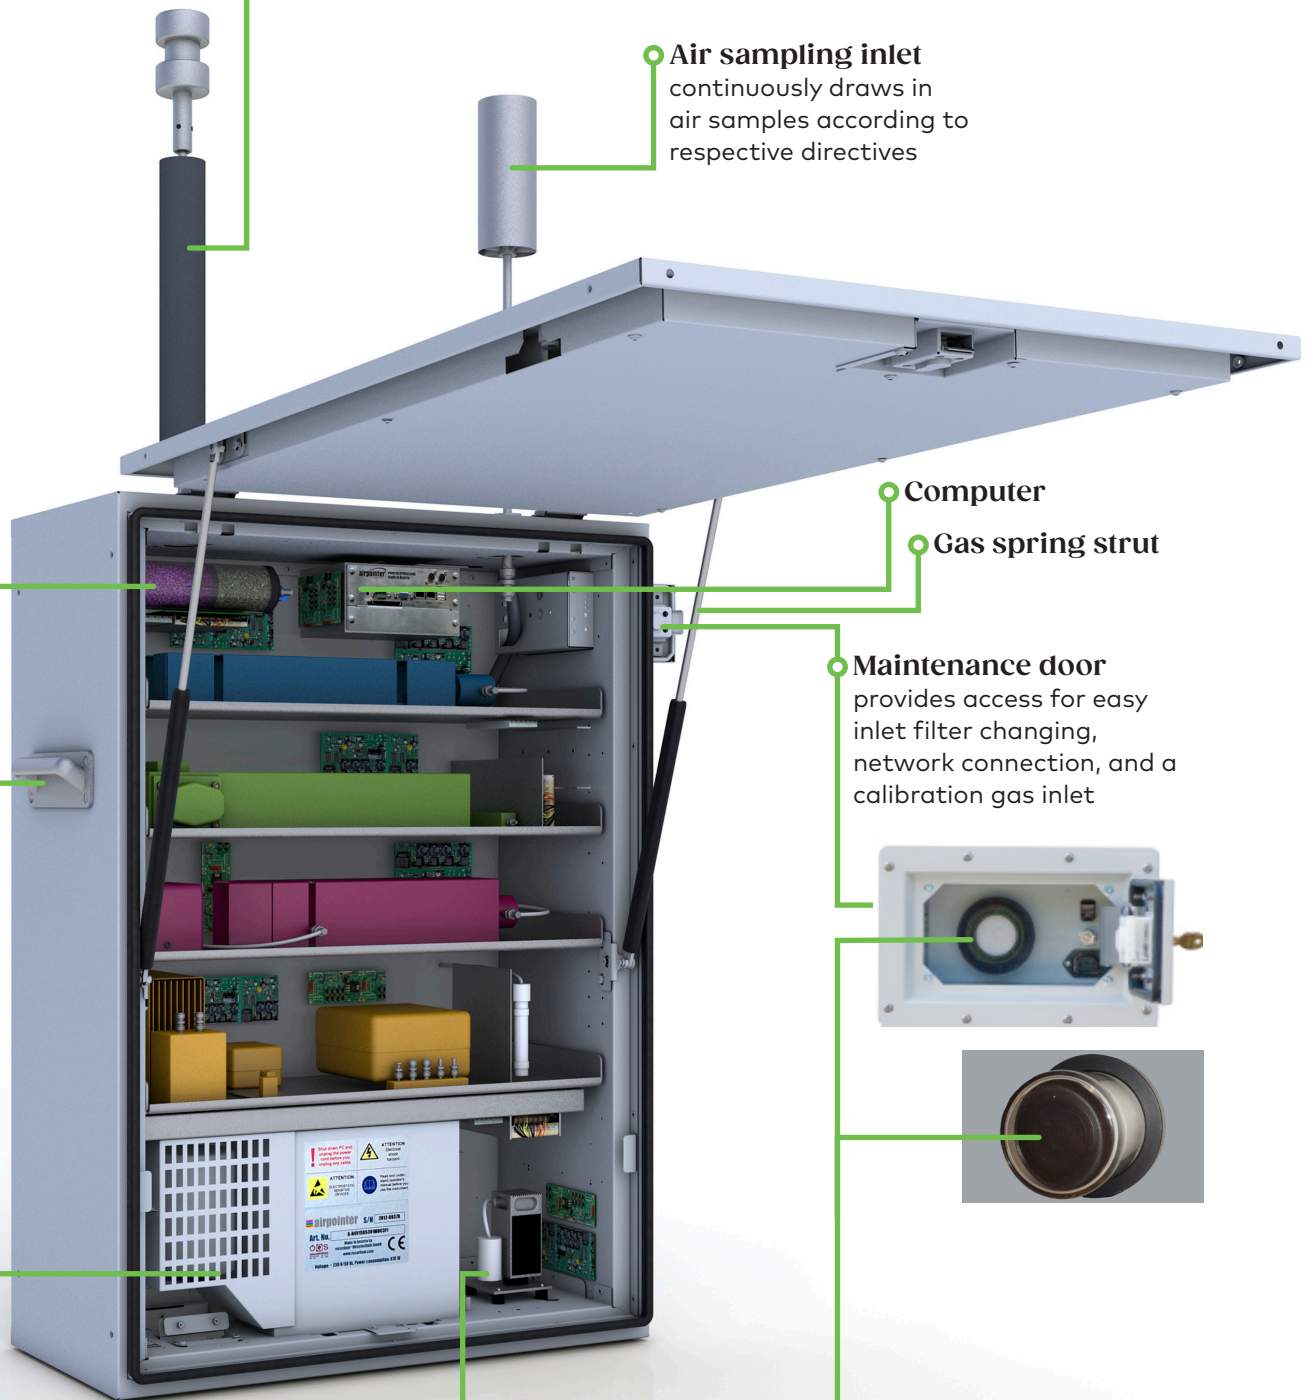



### Airpointer 2D

### Airpointer 4D

### Airpointer PM (HC)


<b>Pollutants standards modules</b>	2 of the following modules	4 of the following modules	4 of the following modules
	NO/NO <sub>2</sub> /NOX	Weight: 12.0 kg / 26.5 lbs, see page 12 for tech. specifications optional: span module	
	O <sub>3</sub> /NOX	Weight: 5.8 kg / 12.5 lbs, see page 13 for tech. specifications optional: span module	
	SO <sub>2</sub> (H <sub>2</sub> S)	Weight: 8.5 kg / 18.7 lbs, technical specifications pages 14–15 optional: span module, H <sub>2</sub> S module	
	CO	Weight: 9.0 kg / 19.8 lbs, see page 16 for tech. specifications optional: span module	
	PM10/PM2.5	Type approved PM10 and PM2.5 (Met One BAM1020 or EDM 180C)	

<b>More sensor Modules</b>	BTX	see page 13 for technical specifications
	Standard Modules Dust Monitoring: Nephelometer for indicative PM monitoring (PM10, PM2.5) or Multi PM (laser spectrometer) for indicative PM monitoring (PM10, PM4, PM2.5, PM1 and TSP)	
	Meteorological sensors: wind direction, wind velocity, temperature, air pressure, relative humidity, precipitation, made by various manufacturers	
	Traffic data sensors: traffic count, made by various manufacturers	
	Noise sensors, made by various manufacturers	
	Electrochemical sensors for formaldehyde, ethane, chlorine... For industrial applications, environmental hygiene, and indoor air quality monitoring (IAQ)	
	Sensors for monitoring indoor CO2 (IAQ)	
Navigation system (GPS) for linking monitoring data with geographical data		

<b>Features (model)</b>			
Dimensions (H/W/D, w/o sample inlets)	890 x 920 x 400 mm / 34.80 x 36.22 x 15.75 in	1120 x 920 x 400 mm / 44.09 x 36.22 x 15.75 in	1480 x 920 x 650 mm / 58.28 x 36.22 x 25.59 in
Weight	65.8 kg / 145.1 lbs	73.9 kg / 162.9 lbs	110 kg / 242.5 lbs
Power consumption*	670 W	max. 670 W	max. 2,000 W
Flow without dust:	< 2,000 ccm/min	< 3,000 ccm/min	< 3,000 ccm/min

<b>Common features</b>	
Construction	Well-isolated double aluminum construction Standard monitoring modules on removable drawers Rugged, inconspicuous burglar-proof design
Standard equipment	Internal air conditioning and temperature control Maintenance door Cylinder lock (standard)
Operating temperatures	Zero air supply -20 °C / -4 °F to +42 °C / 108 °F (optional heating for down to -40 °C / -40 °F) (+50 °C for HC)
Options	Various types of mounting brackets Wireless communication (LTE/UMTS/3G modem,...) Sample gas conditioning (high relative humidity, high PM exposure) Integration of external devices and instruments (e.g. 4 – 20 mA, RS-232, Modbus via IP,...) Solutions to communicate with external data systems (e.g. TCP-IP, Modbus via IP, RS-232, 4 – 20 mA,...) Various base frames and handling devices for on-site operation (roadside, workshop, indoor, pickup truck, trailer,...)



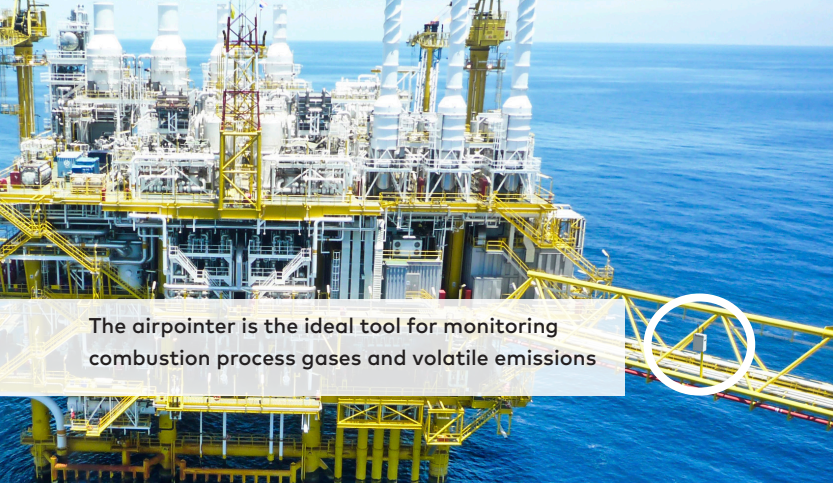

The airpointer is the ideal tool for monitoring combustion process gases and volatile emissions

## Reliable point of interest monitoring


Ambient air quality with regard to health-harming substances also has to be considered on a small scale, because local microclimatic conditions may create an air quality considerably differing from a large-scale approach. Health hazards caused by a momentary pollutant concentration increase indicate the necessity of point of interest monitoring.

## Airpointer in industry and traffic

The airpointer is the ideal tool for monitoring CO, O<sub>3</sub>, H<sub>2</sub>S, SO<sub>2</sub>, NO / NO<sub>2</sub> / NO<sub>x</sub>, PM and BTX, because of its high flexibility. The traffic data sensor is one of many add-on sensors, which may be added quickly and simply. It enables measuring the number of vehicles and their average speed. Resulting data may be recorded and clearly displayed, for example in combination with nitrogen oxide and PM data.



Road traffic-related monitoring with the airpointer, data may be used as control signals for a traffic management system

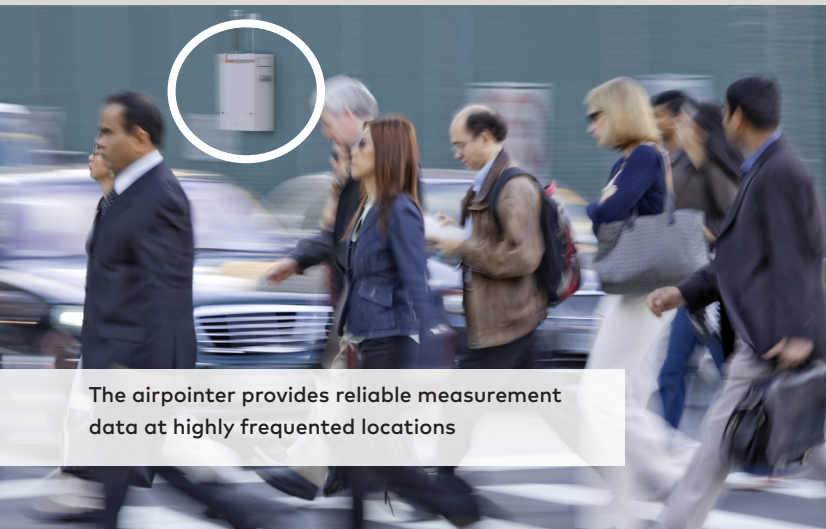

The airpointer provides reliable measurement data at highly frequented locations

## Airpointer at hot spots and indoors

The airpointer measures areas where people frequently stay and poor air quality affects the health of the individual. Mainly highly frequented places as shopping street, traffic junctions or parks and sports grounds with an intense traffic-related air pollution require reliable measurement data because thresholds will often be exceeded.

People spend more than 80 percent of their time indoors. Frequently, indoor air quality is not better than outdoors. Therefore, continuous indoor air quality monitoring is essential considering that the health of young or elderly people or people in poor health above all suffers rapidly under poor indoor air conditions.

***“We can generally choose what we want to eat and drink and where we want to be, but not the air we breathe”***



Air quality monitoring at schools, public buildings, shopping malls, and airports (In-door Air Quality / IAQ)





## Measuring where necessary

Traditionally air quality monitoring stations are as big as building site containers, installed mostly on large-scale sites. Not the airpointer. It can be quickly installed, cost-effectively operated and easily maintained.

### Mobile operation

It is often necessary to measure briefly at different sites. The compact design of the airpointer makes it the ideal tool for mobile operation.

The airpointer ensures flexible air monitoring while using the required reference measurement methods. The airpointer can be quickly transported by car or trailer to the measurement site where it is needed.

### Permanent installation

The airpointer is typically mounted on a pole (or a wall if necessary). Permanent installation is necessary when continuous monitoring over an extended period is required. The airpointer is lifted to the designated position with a crane and mounted with appropriate mounting brackets. It can be relocated within a minimal amount of time.


### Ready for operation within 30 minutes

- **14:00** - Airpointer delivery and crane mounting
- **14:10** - Airpointer is lifted up a lamp-post
- **14:15** - Fastened with special mounting brackets
- **14:20** - Connection to the power supply and initial start up
- **14:30** - Airpointer is ready for operation. Measurement starts and the user may view the initial data using a web browser



### Personalize your airpointer

The airpointer is delivered in an unobtrusive design and can therefore blend in with its surroundings. By designing the front of the airpointer as you like you can purposely make it conspicuous or use it as advertising space.

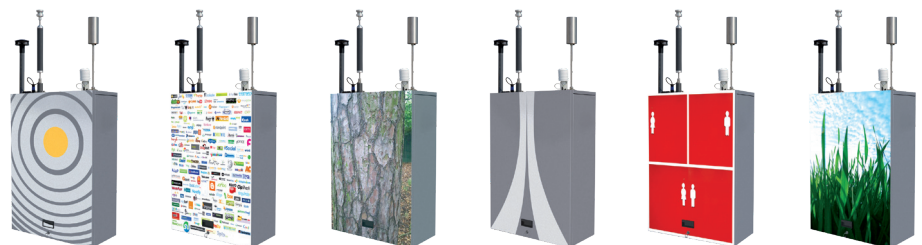





## What is Nitrogen Oxide?

The nitric oxide (NO) molecule is quite reactive and unstable. In ambient air, it reacts with oxygen to form the toxic nitrogen dioxide (NO<sub>2</sub>).

## Where does Nitrogen Oxide come from?

Nitrogen oxide is mainly an unwanted by-product of fuel combustion at high temperatures. Cars and power plants are the main sources of nitrogen oxide.

## What are the effects of Nitrogen Oxide?

Nitrogen oxide causes a multitude of symptoms, primarily in the lungs but also in other organs such as the spleen and liver. Additionally, nitrogen oxide is jointly responsible for acidification and over-fertilization of soil and water. Gaseous nitrogen oxide may become particulate ammonium nitrate. This contributes to large-scale PM (PM<sub>2.5</sub>, PM<sub>10</sub>) pollution. During the summer, nitrogen oxide and hydrocarbons cause formation of ground-level ozone and destruction of the ozone layer.

## Measurement Principle: Chemiluminescence (EN14211)

Nitric oxide in sample gas reacts with ozone to form nitrogen dioxide. This reaction results in electrically excited molecules. These molecules release their excess energy by emitting photons, which are measured by a photomultiplier tube. The airpointer NO<sub>x</sub> module is equipped with a delay loop to measure NO and NO<sub>2</sub> from the same sample.

## Zero air supply check and span point check

Zero air supply is part of the standard equipment so that a zero point check may be carried out automatically (e.g. daily).

An internal NO<sub>2</sub> source for a regular span point check is available as an option.

Measured compound	Nitrogen Oxides NO / NO <sub>2</sub> / NO <sub>x</sub>
EU Directive / USEPA Procedure	Chemiluminescence (EN14211)
Measurement principle	Chemiluminescence
Range	Dynamic, up to 20 ppm
Zero noise	0.2 ppb RMS
Lower detection limit	0.5 ppb
Zero drift (24 hours)	< 0.4 ppb
Span drift (24 hours)	+/- 1% of reading > 100 ppb NO
Response time	< 60 seconds
Precision	1% of reading or 1 ppb (whichever is greater @ < 500 ppb)
Linearity	± 1% of reading > 100 ppb NO
Sample flow rate	1,000 ml/min





## What is Ozone?

Ozone (O<sub>3</sub>) is a highly toxic corrosive substance and a common pollutant. In low concentration it is a normal component of ambient air. Highly concentrated it is an aggressive irritant gas and at ground level it affects humans and nature.

## Where does Ozone come from?

Ozone is formed in the atmosphere by reaction of nitrogen oxides, hydrocarbons, and sunlight. Ozone protects us in higher air layers (stratosphere) from harmful UV radiation. At ground level, higher ozone concentrations form only by other pollutants (ozone precursor chemicals) and sunlight. Nitrogen oxides and volatile organic compounds are the main precursors. Furthermore, methane and carbon monoxide (CO) contribute to the global formation of ozone. Insolation promotes the formation of ozone. High ozone concentrations thus occur mostly at midday and in the afternoon. Major sources of ozone are the chemical processes caused by industry and traffic as well as electrical current of television sets, computers, photocopiers, and electric motors (using brushes).

## What are the effects of Ozone?

Ozone causes above all respiratory ailments such as respiratory syndromes, changes in pulmonary function, increased respiratory sensitivity, and inflammation of the respiratory tract. Ozone additionally destroys the foliage of trees and other plants (photooxidation), thus aggravating the environment.

## Measurement Principle: UV absorption (EN 14625)

A beam from a high-energy UV lamp is directed through a tube filled with sample gas. Absorption effected by ozone is measured with a detector at the end of the tube.

## Zero air supply check and span point check

Zero air supply is part of the standard equipment, so that a zero point check may be carried out automatically (e.g. daily).

An internal ozone generator for a regular span point check is available as an option.

Measured compound	Ozone O <sub>3</sub>
EU Directive / USEPA Procedure	UV photometry (EN14625)
Measurement principle	UV photometry
Range	Dynamic, up to 20 ppm
Zero noise	0.25 ppb RMS
Lower detection limit	0.5 ppb
Zero drift (24 hours)	< 1 ppb
Span drift (24 hours)	± 1% of reading or 1 ppb (whichever is greater)
Response time	< 30 seconds
Precision	1 ppb
Linearity	+/- 1% of reading > 100 ppb O <sub>3</sub>
Sample flow rate	approx. 1,000 ml/min





## What is Sulfur Dioxide?

Sulfur dioxide (SO<sub>2</sub>) is an acid-forming, colorless, foul-smelling and toxic gas.

## Where does Sulfur Dioxide come from?

SO<sub>2</sub> mainly comes from burning coal and heavy fuel oil. Major sources are firing systems in energy business, in industry, and small-scale heating systems that use poor quality sulfurous oil or coal.

## What are the effects of Sulfur Dioxide?

Sulfur dioxide may cause humans to suffer from headaches, nausea, reductions in pulmonary volume, increases in breathing resistance, and symptoms such as wheezing, chest tightness, and shortness of breath. Sulfur dioxide is one of the major "acid rain" precursors which compromises ecological systems such as forests and lakes as well as it accelerates corrosion of buildings and monuments. Sulfur dioxide may reduce visibility as part of smog.

Furthermore, particulate sulfate adds to large-scale PM (PM2.5, PM10) pollution.

## Measurement Principle: UV Fluorescence (EN14212)

Sample gas is lighted with an UV lamp, which causes the SO<sub>2</sub> molecule to absorb energy. The absorbed energy is emitted as a light pulse (photon) which is measured with a photo multiplier.

## Zero air supply check and span point check

Zero air supply is part of the standard equipment, so that a zero point check may be carried out automatically (e.g. daily).

Internal SO<sub>2</sub> sources for a regular span point check are available as an option.

Measured compound	Sulfur Dioxide SO <sub>2</sub> and Hydrogen Sulfide (H <sub>2</sub> S)
EU Directive / USEPA Procedure	UV Fluorescence (EN14212) - for SO <sub>2</sub>
Measurement principle	UV Fluorescence
Range	Dynamic, up to 10 ppm
Zero noise	0.25 ppb RMS
Lower detection limit	0.5 ppb
Zero drift (24 hours)	< 1 ppb
Span drift (24 hours)	± 1% of reading > 100 ppb SO <sub>2</sub>
Response time	< 90 seconds
Precision	1% of reading or 1 ppb (whichever is greater)
Linearity	+/- 1% of maximum > 100 ppb SO <sub>2</sub>
Sample flow rate	500 ml/min



## What is Hydrogen Sulfide?

Hydrogen sulfide ( $H_2S$ ) is a highly toxic and corrosive, nauseously smelling gas.

## Where does Hydrogen Sulfide come from?

$H_2S$  is a gas that results from biodeterioration and biodegradation. Major sources are refineries, furnaces, pulp and paper industry, gasworks, coking plants, sewage plants, and biogas plants.

## What are the effects of Hydrogen Sulfide?

$H_2S$  destroys the body's own hemoglobin and paralyzes oxygen transport in blood. When it comes in contact with mucous membrane, it converts to form alkaline sulfides and causes eye, nose, throat and lung irritations. Its high acidity makes  $H_2S$  a corrosive gas and may cause damage to electronic components.

## Measurement Principle: Thermal conversion to $SO_2$

$SO_2$  is scrubbed from the sample gas.  $H_2S$  is thermally converted to  $SO_2$  and measured by UV fluorescence. Equipped with an  $H_2S$  module the airpointer measures only  $H_2S$  or only  $SO_2$  or both cycling with a minimum switching time of five minutes.

## Zero air supply check and span point check

Zero air supply is part of the standard equipment, so a zero point check may be carried out automatically (e.g. daily).

Internal  $H_2S$  sources for a regular span point check are available as an option.



## Fence line monitoring

Due to its compact size, the airpointer can be mounted around any area and thus be used for small-scale pollutant measuring. Continuous data recording and data transmission enable immediate response in case of varying measurement data. In the event one measuring facility shows increased data, the source of pollution can be pinpointed by taking the wind measurement data into consideration and/or the user's own plant may be ruled out as being the polluter.





## What is Carbon Monoxide?

Carbon monoxide (CO) is an extremely toxic gas resulting from incomplete combustion of carbon and carbonaceous products.

## Where does Carbon Monoxide come from?

Carbon monoxide is mainly a product of incomplete combustion of fuel and propellants. Major sources are traffic, industry and smoking indoors.

## What are the effects of Carbon Monoxide?

CO as pollutant is especially significant because of its toxic effect to humans (damaging hemoglobin). Furthermore CO plays a significant role for photochemical generation of ground-level ozone on a global scale.

A certain concentration may reduce the amount of oxygen received by a person's brain. The person may lose conscience or suffer permanent brain damage caused by lack of oxygen. Carbon monoxide may also contribute towards global warming.

## Measurement Principle: NDIR Gas Filter Correlation (EN14626)

An infrared source beam is directed through a chamber filled with sample gas. Carbon monoxide absorbs this light. A photo-detector measures the emanating decrease.

## CO scrubber check and span point check

A "CO scrubber" (catalytic converter) removes CO from the sample, so a zero point check may be performed automatically (e.g. daily).

An internal CO source for a regular span point check is available as an option.

Measured compound	Carbon Monoxide CO
EU Directive / USEPA Procedure	NDIR gas filter correlation (EN14626)
Measurement principle	NDIR gas filter correlation
Range	Dynamic, up to 1,000 ppm
Zero noise	0.02 ppb RMS
Lower detection limit	0.04 ppb
Zero drift (24 hours)	< .01 ppb
Span drift (24 hours)	± 1% of reading > 10 ppb CO
Response time	< 60 seconds
Precision	± 0.1 ppm
Linearity	+/- 1% of reading < 1,000 ppm CO
Sample flow rate	approx. 500 ml/min



## What is BTX?

Benzene is a clear, colorless, highly flammable and volatile, liquid aromatic hydrocarbon with a gasoline-like odor. Benzene is found in ambient air as a result of burning fuels, such as coal, petrol and wood.

Toluene also known as methylbenzene, is a clear, water-insoluble liquid with the typical smell of paint thinners. It is an aromatic hydrocarbon that is widely used as an industrial feedstock and as a solvent.

Ethylbenzene is an organic compound, it is a highly flammable, colorless liquid with an odor similar to that of gasoline. This monocyclic aromatic hydrocarbon is important in the petrochemical industry as an intermediate in the production of styrene, the precursor to polystyrene, a common plastic material.


Xylene is the term used to describe the three isomers of dimethyl benzene; m-xylene, p-xylene and o-xylene. Xylenes are produced mainly as part of the BTX aromatics (benzene, toluene, and xylenes).

## What are the effects of BTX?

Besides the well-known carcinogenicity of benzene, also the hepatotoxicity, geno toxicity that are risks for human health caused by benzene.

## Zero air supply and span point check

Zero air supply and regular span point check are part of the implemented principle whereas zero and span point check may be carried out automatically on a daily basis.

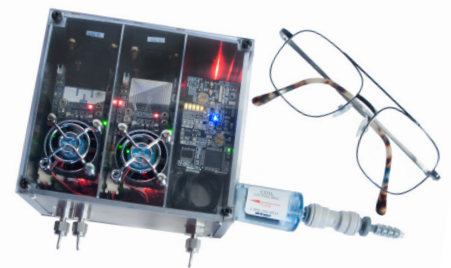

No gas cylinders needed

Measured compound	Carbon Monoxide CO
Analysis time	15 min (15 – 60 min on request)
Standard range	0 – 100 ppb (extended ranges on request)
Detector	PID 10.6eV
Column	MEMS, packed
Oven	Temperature ramp up to 140 °C
Carrier gas	Air, on board generated: < 20 ml/min
Lower detection limit	<0.25 ppb BTEX (each for 15 min analysis time)
Span drift (24hr)	< 3%
Sample flow rate	100-200 ml/min typical





## What is Particulate Matter?

PM10 and PM2.5 are not single components but the mass concentration of all ambient air particles with an aerodynamic diameter smaller than 10  $\mu\text{m}$  (PM10) or 2.5  $\mu\text{m}$  (PM2.5)

## Where does Particulate Matter come from?

Thresholds of these pollutants are frequently exceeded, especially in areas with strong vehicle traffic air pollution. This leads to an increased public awareness of PM issues. Particulate matter comes from diesel exhaust particles, tire wear, brake dust, swirling road dust generated by vehicle traffic, domestic fuel and industrial emissions.

## What are the effects of Particulate Matter?

PM2.5 and PM10 have a short-term effect on the cardiovascular system. Evidence of a direct relation between the number of heart attacks and PM concentration has been substantiated. For instance, a long-term effect of PM pollution is the potential to carry and hold toxic compounds in the respiratory system. Particles in lungs and bronchia weaken the immune system.

### Measurement principle: Nephelometry

The airpointer PM module uses nephelometry, the proven optical method of measurement. A sample heater minimizes the effects of humidity. The module uses a light-scattering photometer with a near-IR LED, a silicon detector hybrid preamplifier and a reference detector. The scattered light is proportional to PM concentration.

**Size selection:** A TSP inlet is part of the standard equipment of the PM module. Simply change the optionally available size-selective inlets to measure PM10 or PM2.5.

Measured compound	Particulate matter
EU Directive / USEPA Procedure	Particle collecting and gravimetric analysis
Measurement principle	Nephelometry
Range	Dynamic, up to 2,500 $\mu\text{g}/\text{m}^3$
Lower detection limit	< 1 $\mu\text{g}/\text{m}^3$
Zero drift (24 hours)	< 1 $\mu\text{g}/\text{m}^3$
Span drift (24 hours)	$\pm$ 1% of reading
Response time	<60 seconds
Precision	1 $\mu\text{g}/\text{m}^3$
Sample flow rate	2 l/min

### Measurement principle: Nephelometry

Particle count to mass conversion provides data of up to five mass ranges simultaneously in one minute. Measured PM mass fractions: TSP, PM10, PM4, PM2.5, PM1

**Number concentration:** up to 8 classes simultaneously (10  $\mu\text{m}$ , 7  $\mu\text{m}$ , 4  $\mu\text{m}$ , 2.5  $\mu\text{m}$ , 1  $\mu\text{m}$ , 0.7  $\mu\text{m}$ , 0.5  $\mu\text{m}$ , 0.3  $\mu\text{m}$ )

Measured compound	Particulate matter
Particle size ranges	TSP, PM10, PM4, PM2.5, PM1
Concentration range	0-1,000 $\mu\text{g}/\text{m}^3$
Sensitivity	0.3 $\mu\text{m}$
Sample duration	1 minute
Sample flow rate	2 l/min




## Airpointer PM (HC)

The airpointer PM (HC) can be equipped with an approved PM analyzer. Furthermore, you may connect the airpointer to an external PM analyzer by using the available interfaces. Thus you may as well use the airpointer's advantages especially within data recording and data transfer for measuring PM.

### Measurement Principle: Laser light scattering

It has the capability to simultaneously measure PM10 and PM2.5 values in real-time, and conforms to European and USEPA standards. More than 30 years of experience in manufacturing of aerosol spectrometers are reflected in the scattered light measurement cell and its electronic signal output for every particle size.

Type approved PM10 and PM2,5  
(Thermo 5030 SHARP, Met One BAM1020 and EDM 180C)

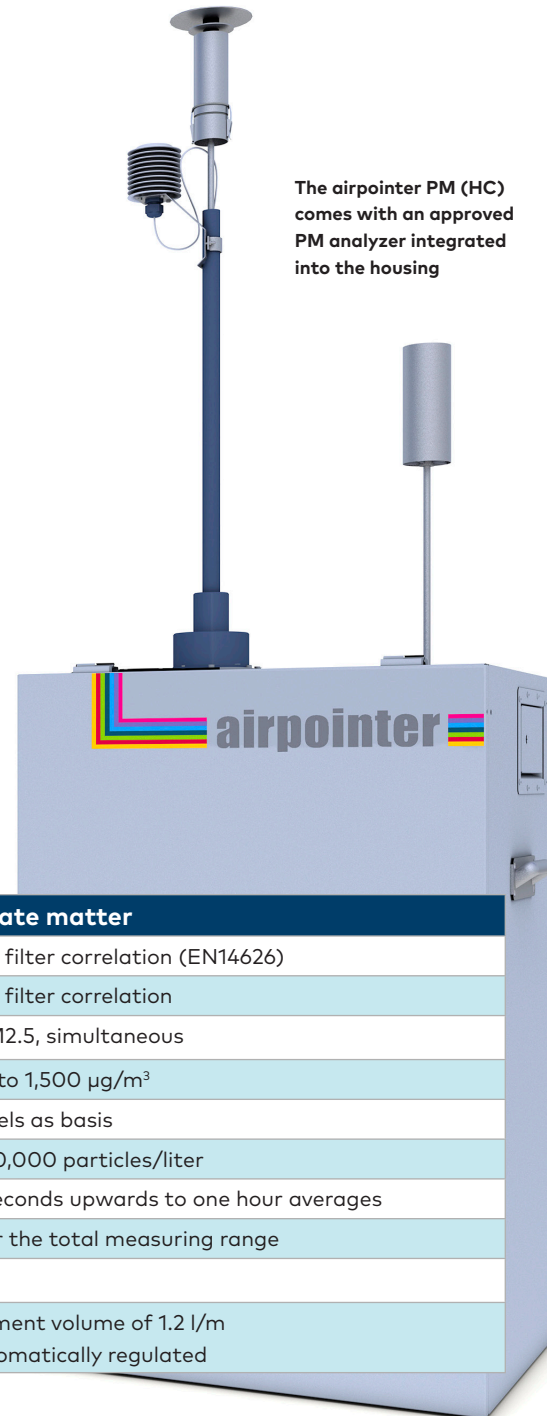

Measured compound	Particulate matter
EU Directive / USEPA Procedure	NDIR gas filter correlation (EN14626)
Measurement principle	NDIR gas filter correlation
PM values	PM10, PM2.5, simultaneous
Range	From 0.1 to 1,500 $\mu\text{g}/\text{m}^3$
Size channels	31 channels as basis
Count range	1 to 3,000,000 particles/liter
Measurement intervals	From 6 seconds upwards to one hour averages
Reproducibility	$\pm 3\%$ over the total measuring range
Laser wavelength	660 nm
Sample flow	Measurement volume of 1.2 l/m $\pm 5\%$ automatically regulated



## Additional airpointer sensors

Apart from the already installed modules the airpointer offers capabilities for implementing additional sensors and external instruments using the high performance airpointer data recording. These sensors are integrated via Ethernet, RS-232 or analog interfaces. Additional sensors are mounted outside or inside the airpointer depending on the space available.

The airpointer continuously manages and controls measurement data via a web based user interface. The high-performance airpointer features can be used for each additionally implemented sensor. This includes data recording over a period of several years, data backup and faster data access via the recordum portal, data download for local analyses and more.

### Additional Sensors

#### Road traffic and public places

- Noise level
- Pedestrian counts
- PM sampling
- PM monitoring
- Navigation systems (GPS)
- UV radiation

#### Industrial hygiene

- Toxic gases
- Volatile organic compounds (VOC)

#### Indoor air quality

- Carbon monoxide (CO<sub>2</sub>)
- Relative humidity
- Temperature
- Light intensity



The meteorological sensor Lufft WS 600 records the parameters wind direction, wind velocity, temperature, air pressure, relative humidity and precipitation.

Next generation air quality monitoring also provides further capabilities for acquiring data. The airpointer is "live on air" at all times and may be accessed by authorized persons via the Internet using a web browser. No special software is necessary. The user may quickly and easily view, download and analyze measurement data, update the data recording system from anywhere in the world and automatically forward maintenance information by email.

### Data access

The user may access data via modem (GSM, GPRS, UMTS) or LAN (direct, cable, or wireless). A separate maintenance interface shows real-time data. The data recording system is also equipped with an interface for communicating with devices made by other manufacturers. Automated downloads allow for data transmission to a central data acquisition system.

### Password protected access

User interface access on various levels requires a login name and is password protected. An optional alarm system sends a text message via SMS in the event of unauthorized access.

### Linux operating system

A Linux-based data processing system guarantees complete Internet connectivity as well as high reliability and flexibility. Data security is provided by an automated internal backup based on a mirrored hard drive.

### What is saved?

**Measurement data:** Depending on the selected modules, data are recorded on an internal hard drive with a minimum storage capacity for five years.


**Operational data:** Temperature of heated and cooled parts, air pressure and fan rotation speed etc. are stored in the database.

### Data backups

Capabilities are provided to also automatically save data to a central server – continuously, so to speak. A network of monitoring systems may also be established using the recordum portal server.




# Airpointer interface

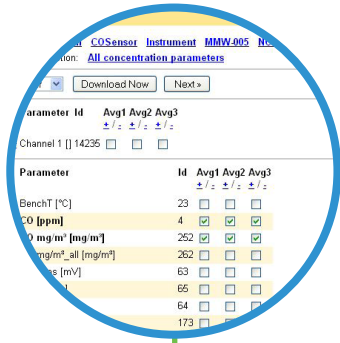

## Download

All parameters can be downloaded easily and quickly to your PC. You may configure the default selection of parameters and use Excel for further processing for example

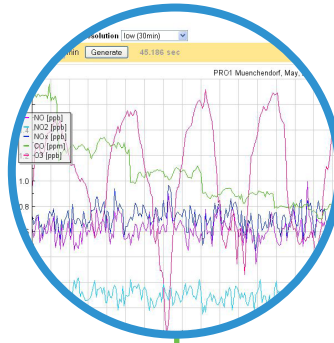


## Measurement data displayed in time diagram

One to six parameters are displayed in a clearly arranged graphic. Zoom function allows for detailed viewing



## Setup

Setup is used for settings in general. Here you may enable or disable the various modules and change units such as ppb and  $\mu\text{g}/\text{m}^3$

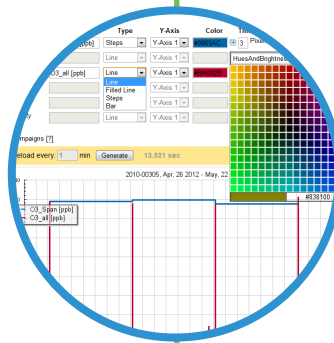


## Graph design

For the purpose of clarity, you may present measurement data in different form and in various colors: as a line, a filled line, a step or a bar diagram



## Measurement campaign

Measurements may be assigned to defined time periods and locations

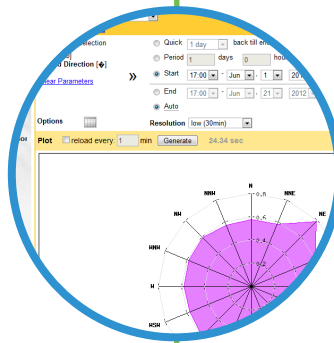

## Radar chart / wind rose


Measurement data may be displayed in relation to wind direction to localize pollution sources

Date	CO [ppm]	NO [ppb]	NO2 [ppb]
15:00:00	0,1	0,4	0,0
15:30:00	0,1	0,0	0,0
16:00:00	0,1	0,7	0,1
16:30:00	0,0	1,3	-0,1
17:00:00	0,1	2,9	-0,1
17:30:00	0,1	2,7	-0,1
18:00:00	0,1	2,2	0,0
18:30:00	0,1	1,4	0,0
19:00:00	0,1	0,7	0,0
19:30:00	0,1	0,7	0,0
20:00:00	0,1	0,6	0,0
20:30:00	0,1	0,6	0,0

## Reports

Reports may be defined and automatically created. The results are converted to pdf or xls files.

## Quality assurance QA/QC

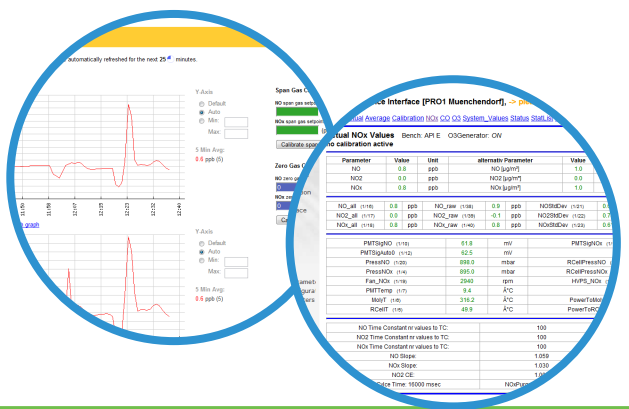

## Many years of security, reliability and continuity

The airpointer has been developed by experts with field experience with special emphasis placed on data quality assurance. recordum quality management is certified for research, development and production in accordance to ISO 9001:2008 standards.

Only a minimum amount of maintenance is necessary to continuously guarantee the quality of the measurement data. The filter, absorbent and zero air cartridge should be checked regularly while the device is operating. The modules and electronics must be checked once a year. The airpointer is equipped with a large number of functions for controlling and maintaining operation, which are easy to use, clearly displayed, and quickly implemented.

## Calibration

A span gas port in the maintenance door is provided for calibrating the airpointer with external span gas. The user does not have to open the front door thus leaving the temperature inside unaltered. The airpointer is calibrated using a graphic interface in the user menu, which displays the parameters to be calibrated in a concentration-time-diagram. Thus the user may evaluate stability of both measurement signal and span gas concentration. After calibration, the airpointer displays a message indicating whether or not the calibration was successful. The calibration data are saved and can be retrieved at any time.

## Software

A user network connection (RJ45) located behind the maintenance door is provided for local operation and monitoring of all device functions. Extensive diagnostic functions included in the software are used to continuously monitor all key operating parameters and save them once a minute in the system data base for preventive fault detection and tracking the effect of faults on measurement data.

A separate program (watchdog) additionally controls correct operation and automatically repairs any faults that may occur. Changes of site, calibrations, faults and their remedies etc. can be entered in an electronic station logbook. You may further increase data security by using an automatic backup with the recordum portal independent of the airpointer.

## Operational test

Each airpointer features internal zero air generation for automatic or manual zero point check of each module. You may individually select a zero point check or an automatic adjustment. You may optionally check all gas ambient air analyzer modules individually using internal span gas generation and the following methods.

### Ozone

An ozone generator generates a constant sample flow of ozone using a UV lamp

### Carbon Monoxide

Span is generated using a refillable calibration gas cylinder and an internal dilution system

### Nitrogen Dioxide, Sulfur Dioxide/ Hydrogen Sulfide, BTX


A permeation tube contains the condensed airborne pollutant in liquid form and releases it at a constant high temperature (ensured by a controlled oven) via a membrane

The user may track at all times the results of the internal operational test that are saved in the airpointer database.

## Filter changing

The filter holder is also located in the vicinity of the maintenance door. The filter holder features a glass plate to check the cleanliness of the filter and if it is properly seated. An optional extended lifetime filter with a greater volume extends the intervals between filter changes and is used in high humidity environments and hot climates. The extended lifetime filter is monitored by the airpointer operating system regarding the degree of contamination and level of the integrated reservoir for moisture. The integrated work flow system will send an alarm in case of a malfunction or overflow.



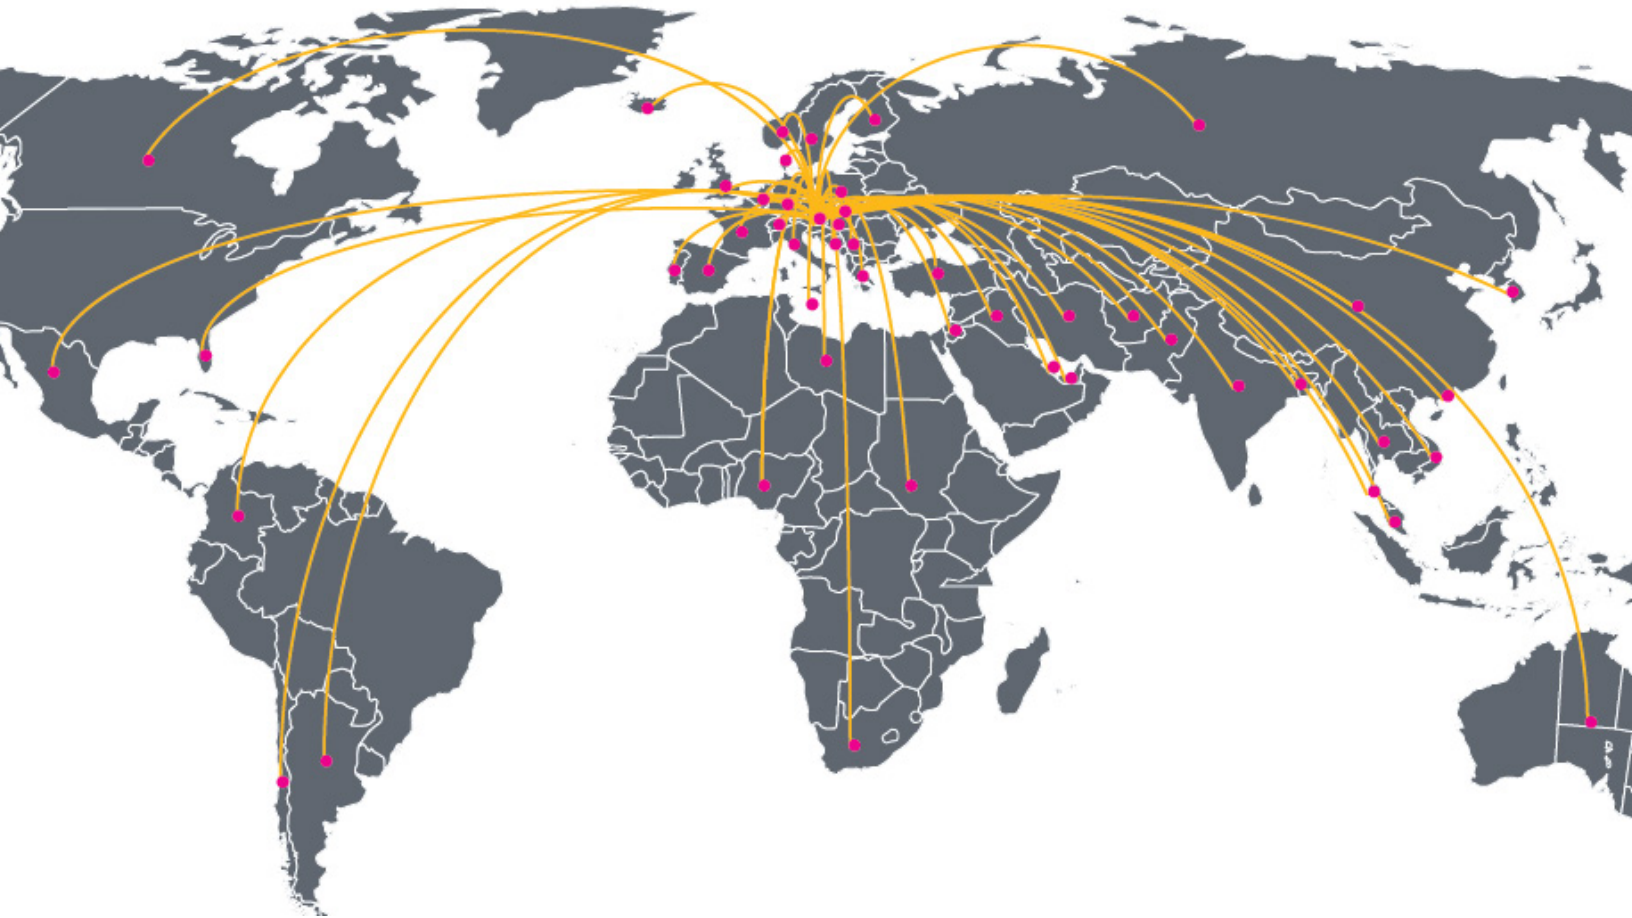

## mlu-recordum - Distribution Network

### Next Generation Air Quality Monitoring

The airpointer is a compact and modularly designed ambient air quality monitoring system for airborne pollutants using internationally defined reference methods that enables you to carry out air quality monitoring at hot spots or other sites with a high ecological relevance. A web browser enables access to clearly arranged graphics of measurement data.

The airpointer is easy to install, cost-effective to operate, and easy to maintain.

In addition to the airpointer, mlu-recordum develops and produces further solutions:

**airQlog** for storing, managing and displaying data of several air quality monitoring instruments and air quality monitoring sensors

**airGrate** for providing precise concentrations of calibration gases and other required gases

**waterpointer** for monitoring water quality

Convenient system solutions for monitoring indoor air quality

## Next generation air quality monitoring

- The airpointer is produced according to ISO 9001:2008 and is subject to continuous enhancement.
- Follows EU directives: EN14625 (O3), EN 14626 (CO), EN 14211 (NO/NO2/NOX), and EN 14212 (SO2) as well as the respective USEPA standards.
- The airpointer's advanced and patented temperature management and energy management systems reduce the power consumption by 90% versus comparable monitoring stations.

[Learn more](#)

**DTN<sup>o</sup>**